




**Enforcer**

## Enforcer Instruction Sheet

1. Ensure the instrument is switched on and is showing the normal monitoring display.
2. If it is not already fitted, screw the Zellweger Analytics cylinder in tightly (part number 2302D0833), check that the pressure gauge shows gas pressure is present, and pull back the instrument drawer.



3. Insert the instrument, by tilting at a slight angle, so that the instrument front cover locks under the lip in the Enforcer as indicated.

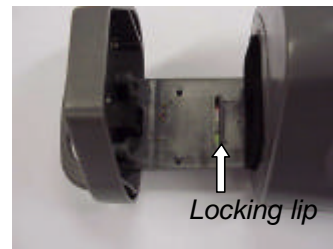

4. Then return the instrument to the vertical. The rear locking mechanism of the Enforcer will retain the instrument. Now close the drawer firmly.



5. The instrument will recognise the Enforcer and display an instruction to press the ✓ button to continue.



Rear Locking catch

6. After about 90 seconds the instrument will display either a pass or fail.
7. If the instrument reports a failure then check that the gas cylinder has sufficient pressure. Then repeat once more. Note that the instrument drawer must be opened and then closed to reactivate the Enforcer. If a subsequent failure should occur please have the instrument serviced and calibrated, as it may be due to blocked or dirty filters, or the sensor(s) has failed.
8. When completed and successful remove the instrument by pressing downwards on the rear locking catch and lifting the instrument out. The instrument will activate all its gas alarms as it detects the gas from the cylinder, and thereby also performing a bump test. The cylinder should be removed after use.

**Find out more**

[www.honeywellanalytics.com](http://www.honeywellanalytics.com)

**Customer business centre  
Europe and the rest of the world**

Honeywell Analytics AG  
Wilstrasse 11-U11  
CH-8610 Uster  
Switzerland  
Tel: +41 (0)1 943 4300  
Fax: +41 (0)1 943 4398  
[sales@honeywellanalytics.co.uk](mailto:sales@honeywellanalytics.co.uk)

**Customer business center  
Americas**

Honeywell Analytics Inc.  
400 Sawgrass Corporate Pkwy  
Suite 100  
Sunrise, FL 33325  
USA  
Tel: +1 954 514 2700  
Toll free: +1 800 538 0363  
Fax: +1 954 514 2784  
[sales@honeywellanalytics.com](mailto:sales@honeywellanalytics.com)

[www.honeywell.com](http://www.honeywell.com)

**Please Note:**

While every effort has been made to ensure accuracy in this publication, no responsibility can be accepted for errors or omissions. Data may change, as well as legislation, and you are strongly advised to obtain copies of the most recently issued regulations, standards, and guidelines. This publication is not intended to form the basis of a contract.  
© 2005 Honeywell Analytics

Issue 2 12/2005  
H\_MAN0613\_V1  
© 2005 Honeywell Analytics

**Honeywell**